

Fig.1

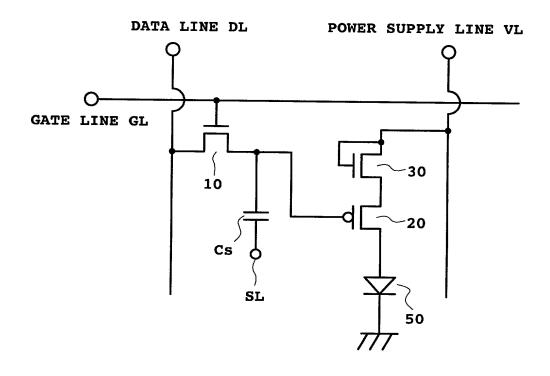


Fig.2

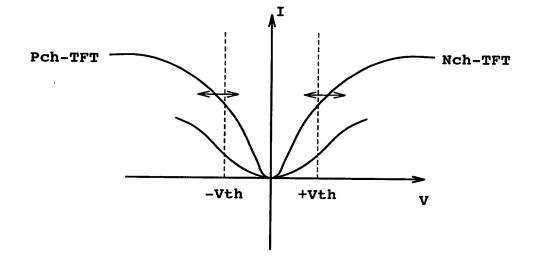
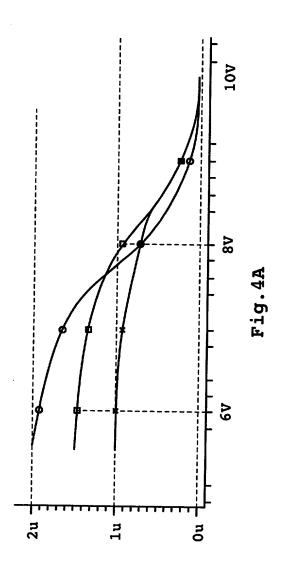


Fig.3



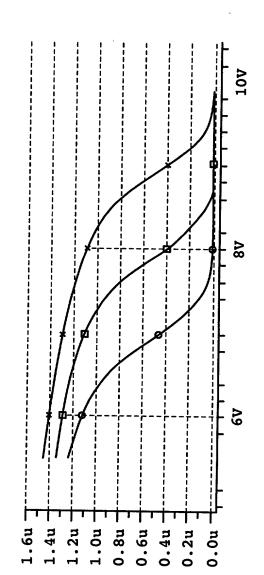


Fig.4B

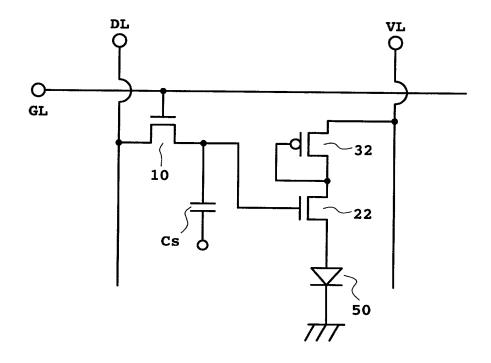


Fig.5

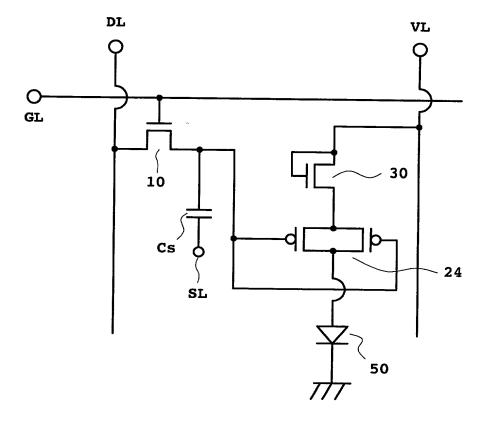


Fig.6

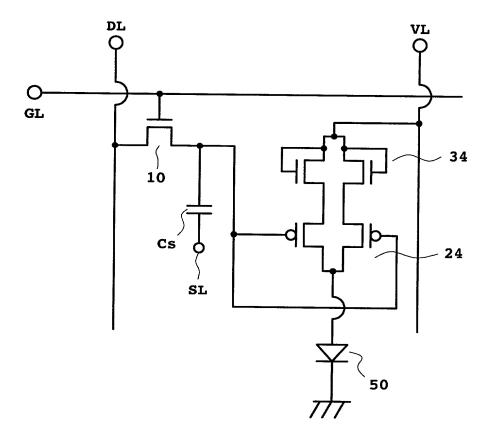


Fig.7

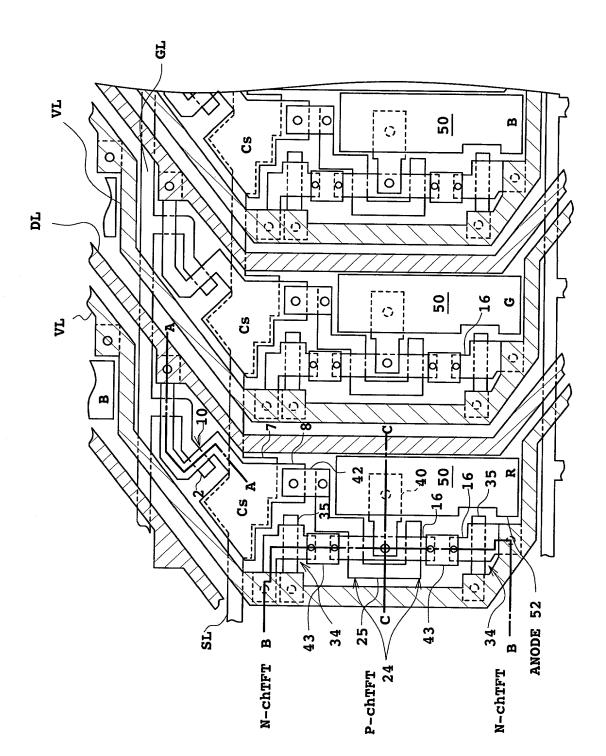


Fig.8

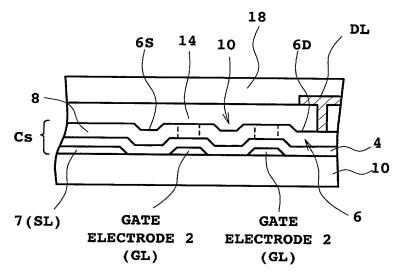
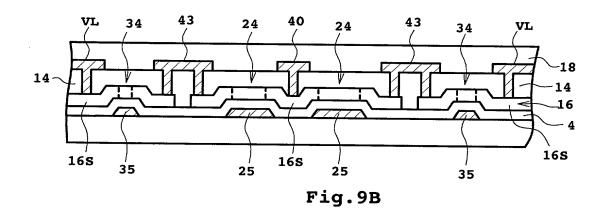


Fig.9A



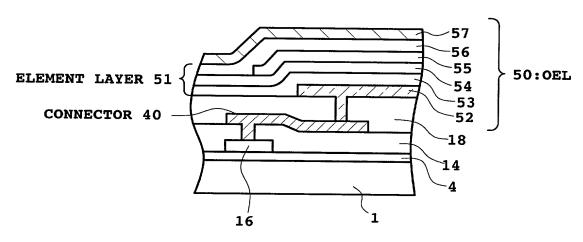


Fig.9C

SCAN DIRECTION OF LASER ANNEAL

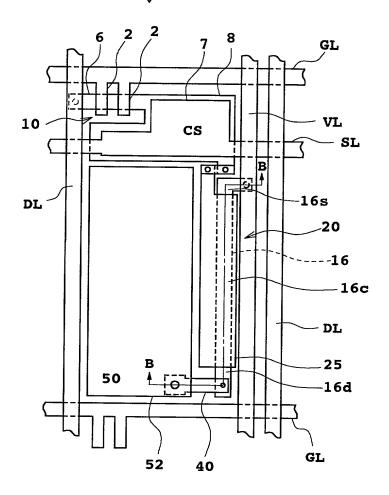


Fig. 10A

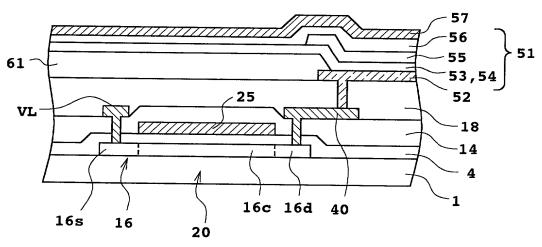


Fig. 10B

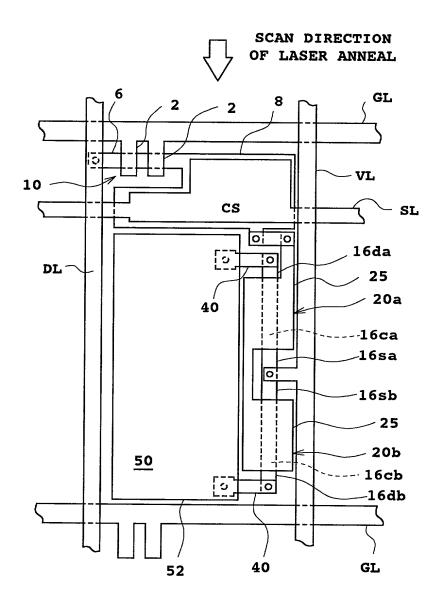


Fig.11

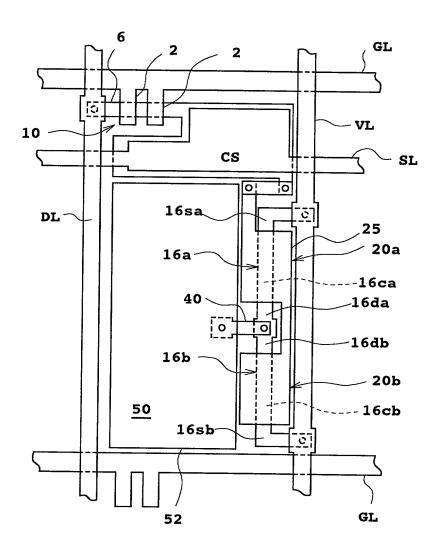


Fig.12

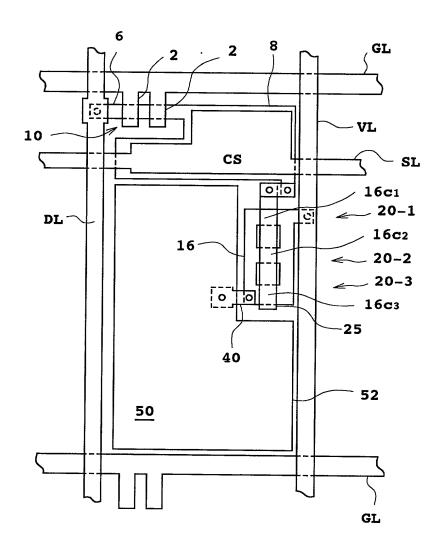


Fig.13

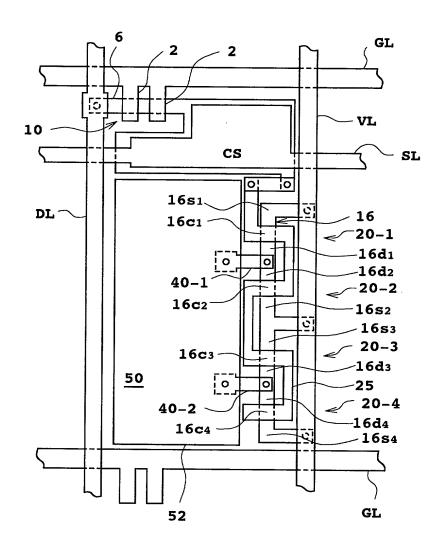


Fig.14

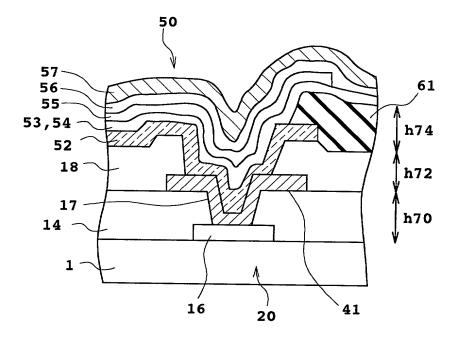


Fig.15A

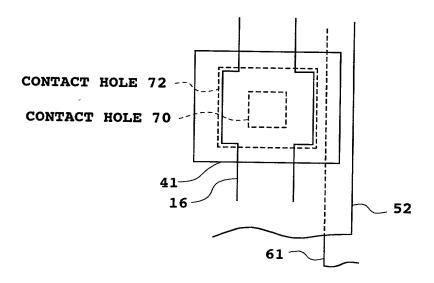


Fig.15B

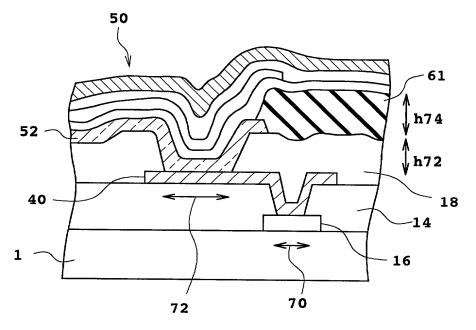


Fig.16A




Fig.16B

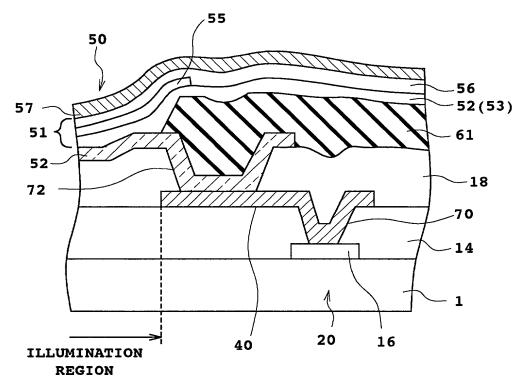


Fig.17

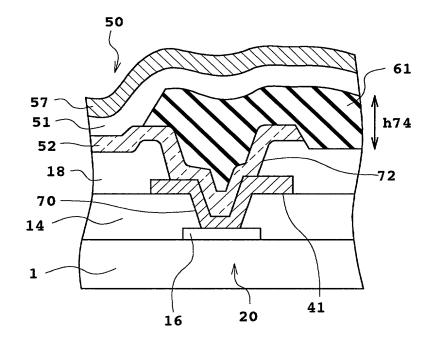


Fig.18

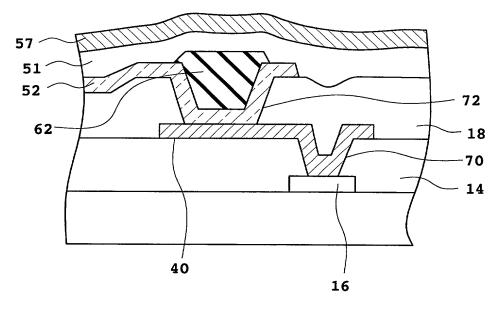


Fig.19

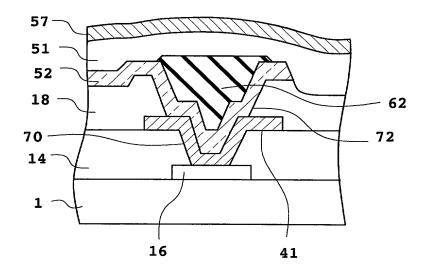


Fig.20